
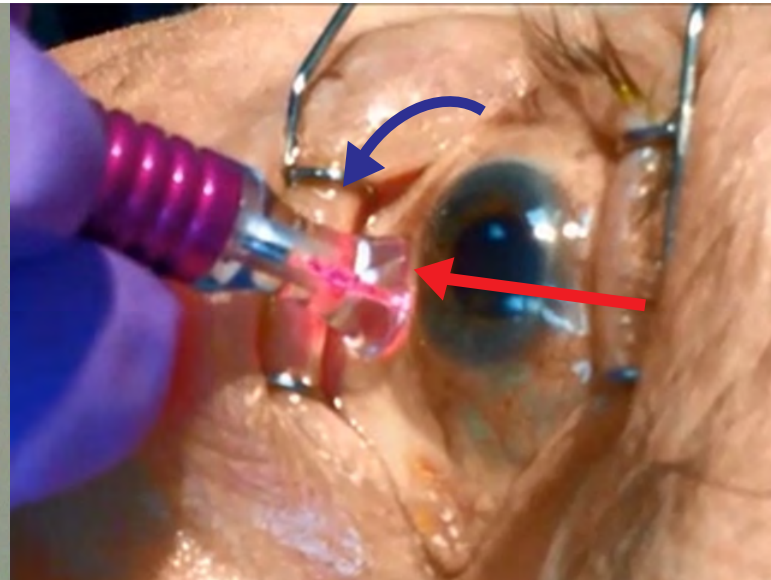


Proper MicroPulse P3 Positioning

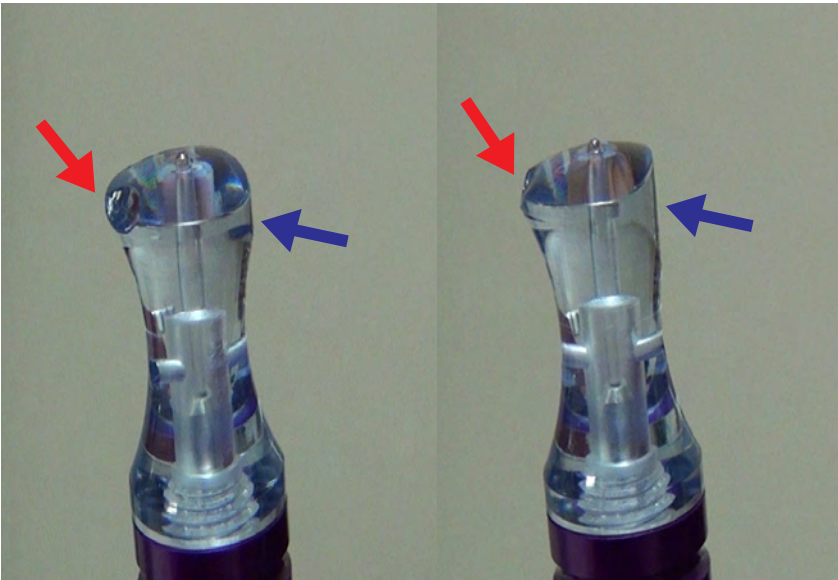

Notch toward the limbus
Flat Side toward the eyelid